Users Guide for the "Medi Hook" Cable Support

- The Medi Hook can be used to raise the cables i.e from active mattresses, off the floor to reduce the likelihood of them becoming trapped.

- A minimum of four hooks are required down the side of the bed, the number can be increased depending on the size, weight and number of cables.

- **Parts of the hook**

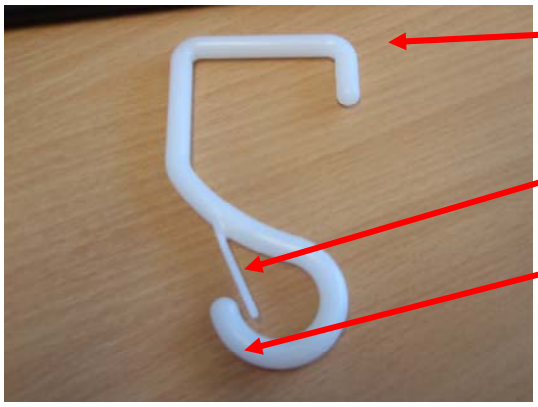

A - Upper part of the hook clips over the bed rail

B - Spring clip to hold the cables in place

C - Lower part of the hook to thread the cables through

- Raise the cotsides (if applicable) to the upright position

- The hooks should be hooked over the bed rail, one at the top, one at the bottom and the remaining positioned evenly between the two.

- Thread the cables through the lower part of the hook

❖ **Cleaning**

Hooks should be wiped down between use with a soft cloth moistened with a mild detergent (or hospital's recommended cleaning solution) and diluted in hot water. Rinse down with clean water and dry off with a paper towel. If any body fluids have been in contact or if the bed has been used by a patient with a known infection, the above procedure should be followed by an additional clean with a chlorine based product as per the trust decontamination policy.

❖ **Please Note**

- When you first use the hook and apply pressure to the spring clip a white mark may appear at the top of the clip but the hook is still suitable for use.